

# AFBR-S10EB001Z

## Evaluation Kit for the AFBR-S10TR001Z Sensor Transceiver



### Application Note 5594

#### Introduction

This application note introduces the evaluation kit AFBR-S10EB001Z, which has been designed to be used as an evaluation platform for the Sensor Transceiver AFBR-S10TR001Z. This evaluation kit provides system designers with a convenient means to evaluate the performance of the AFBR-S10TR001Z sensor transceiver.

The document describes in detail the board included in the evaluation kit and the test setups used for the evaluation of the optical and electrical characteristics of the Sensor Transceiver AFBR-S10TR001Z.

Figure 1 shows the top view of the evaluation board of AFBR-S10TR001Z.

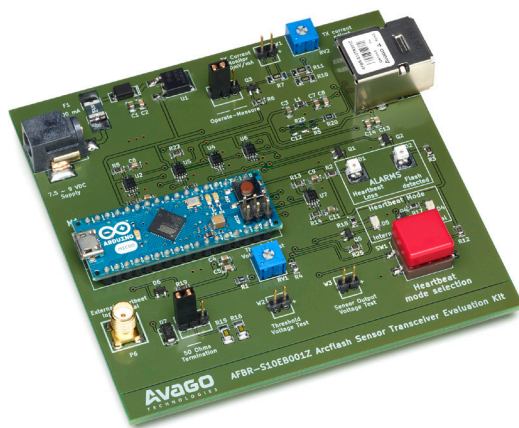


Figure 1. Top side of the evaluation board of AFBR-S10TR001Z

#### Evaluation kit

The evaluation kit includes:

- 1x Evaluation board
- 1x 9.0V DC power supply
- 2x Jumpers
- 1x 1-meter-long AFBR-TUS500Z transparent-jacket-POF patch-chord with AFBR-4526Z duplex connector at its ends (intended for testing of evaluation board in loop configuration).
- 1x 1-meter-long transparent-jacket-POF patch-chord with AFBR-4531Z simplex connectors at its ends
- 1x VL-to-VL AFBR-4536EZ duplex bulkhead
- 2x AFBR-4526Z duplex connectors

The evaluation kit does not include:

- Flash light source \*
- Digital multimeter
- Optical power meter
- Pulse/Pattern generator
- Oscilloscope
- High-impedance probe

\* Any Xenon-based photo camera flash light source is suitable. (Unomat B24 is recommended due to it being commonly available)

## PCB Description

The most important components of the evaluation board are listed below:

- 1x AFBR-S10TR001Z module:  
This device, identified as U3, is the sensor transceiver and, therefore, it is the core of the evaluation board.
- 1x Arduino microcontroller board:  
This device, identified as M1, is the arithmetic-logic unit (ALU) of the evaluation board, where the electrical output of the receiver of AFBR-S10TR001Z is processed. After processing this electrical output, the Arduino microcontroller decides whether the received light has been generated by an arc flash event or, on the other hand, it is due either to a heartbeat sent by the transmitter of AFBR-S10TR001Z or to ambient light.
- 1x switch button:  
This switch button, identified as SW1, allows the user choosing the desired heartbeat mode. The possible options are Internal Heartbeat Mode and External Heartbeat Mode.
- 1x SMA connector:  
This connector, identified as P6, allows the user providing an external heartbeat signal to the sensor transceiver. The aim of the heartbeat signal is to periodically check the availability of the arcflash detection system, including the sensor transceiver (AFBR-S10TR001Z) and the sensor fiber (AFBR-TUS500Z).
- 2 x 3-pin headers:  
One of the 3-pin headers, identified as JP1, allows enabling/disabling a  $50\Omega$  termination, which is placed between the SMA connector previously mentioned and ground. The aim of the  $50\Omega$  termination is to provide impedance matching in case that the external heartbeat signal is supplied from an external pulse/pattern generator with this output impedance; the second 3-pin header, identified as JP2, is used to configure the operation mode of AFBR-S10EB001Z. There are two possible operation modes: Operate and Measure. These two modes of operation are described in the next section of this application note. To enable/disable the  $50\Omega$  termination by means of JP1 and/or to select Operate mode/Measure mode by means of JP2, the user has just to shortcircuit the appropriate pins of the 3-pin headers JP1 and/or JP2 by placing a jumper on them. The required jumpers are provided with the evaluation kit.

- 3 x 2-pin header:  
One of the 2-pin headers, identified as W1, allows monitoring the forward current of the transmitter of AFBR-S10TR001Z (this current is monitored through R7, as shown in the schematic depicted in Figure 8); the purpose of the second 2-pin header, identified as W2, is to monitor the threshold fixed to differentiate between the heartbeat signal or noise generated either by ambient light or by the receiver of AFBR-S10TR001Z itself; finally, the third 2-pin header, identified as W3, allows sensing the output voltage generated by the receiver. To monitor the forward current of the transmitter of AFBR-S10TR001Z, by means of the 2-pin header W1, and/or to monitor the threshold fixed to differentiate between the heartbeat signal or noise, by means of the 2-pin header W2, a digital multimeter properly connected to said 2-pin headers is needed.
- 2x potentiometer:  
One of the potentiometers, identified as RV1, allows changing the level of the threshold used by the Arduino microcontroller to distinguish between heartbeat signal and noise; the other potentiometer, identified as RV2, allows modifying the forward current through the LED of the transmitter of AFBR-S10TR001Z, which is translated into a modification of the optical power of the heartbeat signal of the system (as mentioned before, the forward current of the transmitter of AFBR-S10TR001Z may be monitored by means of the 2-pin header identified as W1). To modify the values of the potentiometers RV1 and/or RV2, the use of the appropriate screwdriver is required.

Figure 8 shows the schematic of the evaluation board supplied in the AFBR-S10EB001Z evaluation kit.

## AFBR-S10TR001Z Transmitter

The transmitter of AFBR-S10TR001Z provides the system with the capability of sending a heartbeat signal to the receiver of said device, which makes it possible to periodically auto-test the arc flash detection system. The transmitter consists of a bare LED, which is driven by an electrical current. This electrical current may be adjusted by means of the potentiometer RV2, allowing a variation in the LOP of the transmitter ranging from -1dBm (peak) to -18dBm (peak). The 2-pin header W1, which is connected in parallel to a 10Ω resistor, makes it possible to monitor the LED driving current. When the LOP of the transmitter is -1dBm, the voltage drop measured at the 2-pin header W1 is 310mV (31mA), while this voltage drop is 7mV (700μA) when the LOP of the transmitter is -18dBm.

To monitor the LOP it is necessary to connect the transmitter of AFBR-S10TR001Z to an optical power meter by means of the 1-meter-long transparent-jacket-POF patchcord with AFBR-4531Z simplex connectors supplied with the evaluation kit AFBR-S10EB001Z.

To facilitate the adjustment of the optical power launched by the transmitter of AFBR-S10TR001Z, the 3-pin header JP2 permits switching between pulsed LED driving current (Operate mode) or continuous LED driving current (Measure mode), which is translated into pulsed output light or continuous output light. Therefore, for the adjustment of the optical power launched by the transmitter, it is recommended to select Measure mode at JP2. When this mode is selected, the optical power measured at the output of the transmitter will be given in terms of peak values. Once the desired peak value is reached by tuning the potentiometer RV2, the mode selected at JP2 is changed from Measure to Operate, which will change the light generated by the LED from continuous wave (CW) to pulsed wave.

## AFBR-S10TR001Z Receiver

The receiver of AFBR-S10TR001Z consists of an ASIC which implements the functionalities of a photodetector plus a trans-impedance amplifier (TIA). The ASIC generates a voltage output whose amplitude is proportional to the power of the received light.

The evaluation board allows the user to adjust the threshold of the heartbeat signal detection. The adjustment is made through the potentiometer RV1 and allows setting a value for the output voltage of the receiver of AFBR-S10TR001Z below which the Heartbeat Loss alarm is triggered. When this alarm is triggered, the LED D1 brightens. The lower limit at which the heartbeat detection threshold

may be fixed is 30mV, while the upper limit at which this threshold may be fixed is 4V. It is important to remark that, when it comes to triggering the Heartbeat Loss alarm, the output voltage of the receiver of AFBR-S10TR001Z is evaluated only inside the time window in which the heartbeat pulse is expected; therefore, it does not matter what said output voltage is outside the mentioned time window (see Figure 2 for clarification).

In the case of the threshold used for the detection of arc flash events, it is hardcoded in the Arduino microcontroller. This threshold is 20mV, which means that if the output voltage of AFBR-S10TR001Z is above this value, the Flash Detected alarm is triggered. When this happens, the LED D2 brightens. As in the previous case, it is important to remark that, when it comes to triggering the Flash Detected alarm, the output voltage of the receiver of AFBR-S10TR001Z is evaluated only outside the time window in which the heartbeat pulse is expected; therefore, it does not matter what said output voltage is inside the mentioned time window (see Figure 2 for clarification).

## Microcontroller

The differentiation between an arc flash event, heartbeat signal and ambient light is made through the Arduino microcontroller placed on the evaluation board. To achieve this differentiation, the microcontroller evaluates the output of the receiver of AFBR-S10TR001Z inside and outside a time window of certain duration.

Figure 2 shows a schematic of the time window referred in the previous paragraph.

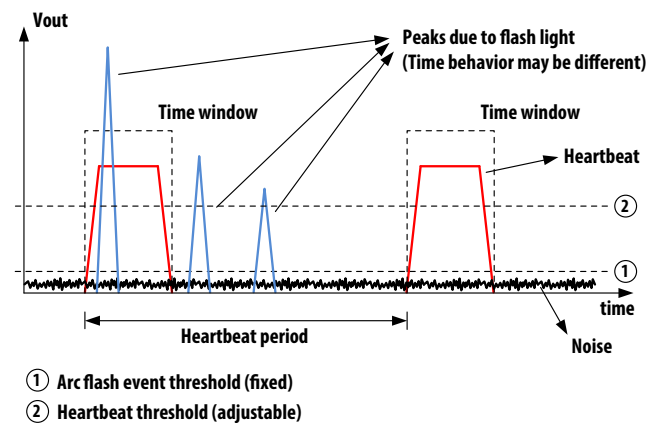


Figure 2. Schematic of the time window implemented in the Arduino microcontroller placed on AFBR-S10EB001Z

According to Figure 2, the following cases may occur:

- The receiver generates an output inside the time window whose amplitude is above the threshold set by means of RV1: in this case, the microcontroller determines that a heartbeat pulse has been received. The Heartbeat Loss alarm is not triggered. The Flash Detected alarm is not triggered either, since this alarm cannot be triggered within the time interval enclosed by the time window.
- The receiver generates an output inside the time window whose amplitude is below the threshold set by means of RV1: in this case, the microcontroller triggers the Heartbeat Loss alarm and, consequently, turns the LED D1 on. The LED D1 will remain on until the amplitude of the output generated by the receiver inside the time window is above the threshold set by means of RV1.
- The receiver generates an output outside the time window whose amplitude is above 20mV: in this case, the microcontroller triggers the Flash Detected alarm and, consequently, turns the LED D2 on, which will remain in this state for 4 seconds. In order to let the user visualize the Flash Detected alarm, any activity of the board is paused during these 4 seconds.
- The receiver generates an output outside the time window whose amplitude is below 20mV: in this case, the microcontroller determines that no arc flash event has occurred. The Flash Detected alarm is not triggered.

In addition to the differentiation between arc flash events, heartbeat pulses and pure noise, the Arduino microcontroller may also produce the electrical signal used to drive the transmitter of AFBR-S10TR001Z and generate the optical heartbeat pulses. When the Internal Heartbeat Mode is chosen by means of the switch button SW1, the Arduino microcontroller generates one 50µs-long pulse each second.

### SMA connector (P6)

The SMA connector placed on the evaluation board allows the user to supply an external heartbeat signal to the transmitter of AFBR-S10TR001Z.

The External Heartbeat Mode, can be enabled by pressing and holding the switch button SW1 until the LED D4 is on. If the output impedance of the pattern/pulse generator used to produce the external heartbeat signal is 50Ω, which is the general case, this impedance must be selected by means of the 3-pin header JP1.

Table 1 shows the characteristics that the external heartbeat signal must have.

**Table 1. External heartbeat signal characteristics**

|                     |               |
|---------------------|---------------|
| High Voltage Level  | 3.5V to 5.0V  |
| Low Voltage Level   | 0V to 1.5V    |
| High level duration | 100µs to 1ms  |
| Repetition rate     | 0Hz to 1000Hz |

### Sensor Output Voltage Test (W3)

This 2-pin header allows the user monitoring the output voltage of AFBR-S10TR001Z by means of an oscilloscope and a high-impedance probe.

## Test setups

This section explains in detail the basic test configurations that may be used to evaluate AFBR-S10TR001Z sensor transceiver by means of the evaluation board provided in the AFBR-S10EB001Z evaluation kit.

### Normal operation

Figure 3 shows the configuration for normal operation of the evaluation board.

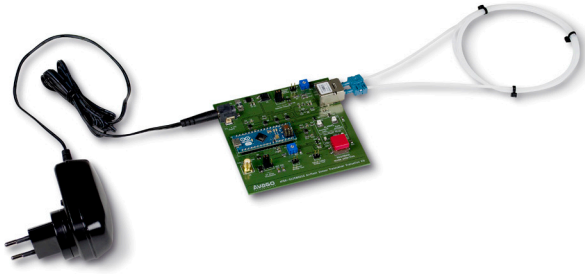


Figure 3. Configuration for normal operation of the evaluation board

In this configuration, the electrical heartbeat signal is internally generated by the Arduino microcontroller and it is later translated into the optical domain by the transmitter of AFBR-S10TR001Z. The optical heartbeat signal travels inside the core of the transparent-jacket-POF patch-cord and reaches the receiver of the AFBR-S10TR001Z within the time window specified for that purpose. The amplitude of the electrical signal generated by the receiver due to the optical heartbeat signal is above the heartbeat detection threshold which has been set by means of the potentiometer RV1; therefore, the Arduino microcontroller does not trigger the Heartbeat Loss alarm and the LED D1 remains off. No flash light is generated, which makes the LED D2 to remain off as well.

Figure 4 shows the electrical output generated by the receiver of AFBR-S10TR001Z, which is available at the 2-pin header W3 and has been monitored by means of a high-impedance probe connected to an oscilloscope.

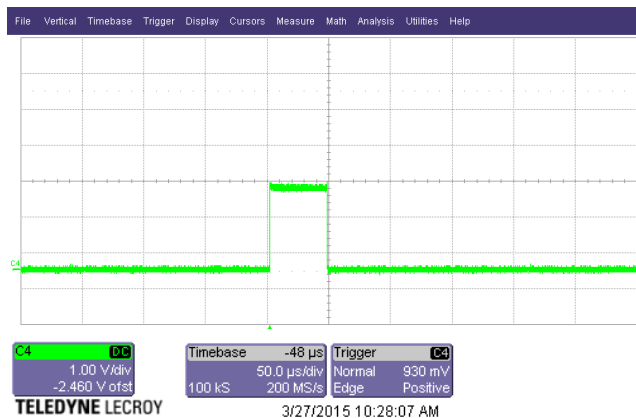


Figure 4. Electrical output available at the 2-pin header W3 for normal operation of the evaluation board

### Heartbeat loss

Figure 5 shows the configuration used to test the Heartbeat Loss alarm implemented in the evaluation board of AFBR-S10TR001Z.

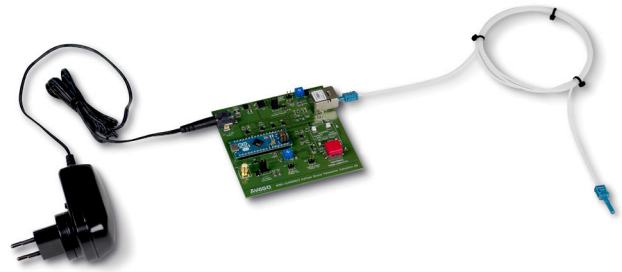


Figure 5. Configuration used to test the heartbeat loss alarm of the evaluation board

In this configuration, as in the previous one, the electrical heartbeat signal is internally generated by the Arduino microcontroller and later translated into the optical domain by the transmitter of AFBR-S10TR001Z. However, since the transparent-jacket-POF patch-cord has been disconnected from the receiver, the heartbeat signal cannot be detected, which makes the Arduino microcontroller to trigger the Heartbeat Loss alarm and to turn the LED D1 on.


The same result would be obtained if, instead of disconnecting the transparent-jacket-POF patch-cord from the receiver of AFBR-S10TR001Z, the potentiometer RV1 was set to a value which fixed a heartbeat detection threshold above the level of the output voltage generated by the receiver of AFBR-S10TR001Z when a heartbeat pulse is received.

In the same way, the Heartbeat Loss alarm would be triggered as well if, by means of the potentiometer RV2, the optical power of the heartbeat pulses was set to a value low enough as to make the receiver of AFBR-S10TR001Z to generate an electrical output below the threshold fixed for the heartbeat detection by the potentiometer RV1.

In conclusion, the Heartbeat Loss alarm may be triggered by either disconnecting the transparent-jacket-POF patch-cord from the receiver of AFBR-S10TR001Z or by fixing the potentiometers RV1 and/or RV2 to the appropriate values.

## Arc flash event detected

Figure 6 shows the configuration used to test the Flash Detected alarm implemented in the evaluation board of AFBR-S10TR001Z.

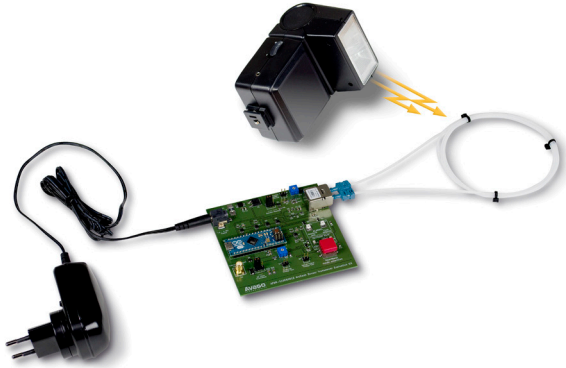


**Figure 6. Configuration used to test the arc flash event detection alarm of the evaluation board**

In this configuration, the electrical heartbeat signal is externally generated by a pulse/pattern generator. The reason for changing from internal heartbeat generation to external heartbeat generation is that the period of the heartbeat signal, when internally generated, is 1s, which is too long if, as in this case, it is desired to have a few heartbeat pulses together with the arc flash event visualized on the screen of the oscilloscope, as shown in Figure 7.

The heartbeat signal generated by the pulse/pattern generator is translated into the optical domain by the transmitter of AFBR-S10TR001Z. This optical heartbeat signal travels inside the core of the transparent-jacket-POF patch-cord and reaches the receiver of AFBR-S10TR001Z within the time window specified for that purpose.

By means of the flash light source, a flash light, which emulates an arc flash event, is generated. When the high optical power of the flash light reaches the receiver of AFBR-S10TR001Z, it generates an electrical output whose amplitude should be above the 20mV threshold fixed for the detection of arc flash events. If this is the case, the Arduino microcontroller will determine that an arc flash event has occurred, triggering the Flash Detected alarm and turning the LED D2 on. This LED will remain on for 4 seconds.

Figure 7 shows the electrical output generated by the receiver of AFBR-S10TR001Z when an arc flash event is detected. This output is available at the 2-pin header W3 and has been monitored by means of a high-impedance probe connected to an oscilloscope.

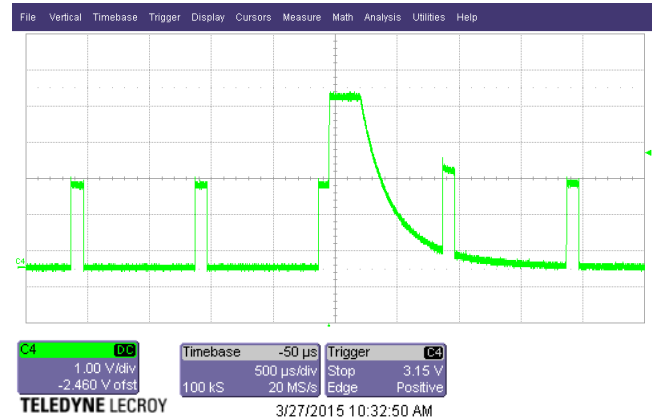

**Figure 7. Electrical output available at the 2-pin header W3 of the evaluation board when an arc flash event is detected**

As may be observed in Figure 7, the arc flash event duration is longer than one heartbeat pulse, which assures that the Flash Detected alarm would be triggered even in the case that the arc flash event started at the same time as the heartbeat pulse.

## IMPORTANT NOTE!

Both external and internal heartbeat generation may be set for any of the three test setups previously described. However, the user must select the desired heartbeat mode by means of the switch button SW1 prior to checking any of the three test setups.

## Evaluation board schematic and bill of materials (BOM)

The bill of materials (BOM) of the board included in the evaluation kit AFBR-S10EB001Z is given in Table 2. The electrical schematic of the evaluation board is shown in Figure 8.

**Table 2. Bill of materials**

| Component        | Description          | Value         | Package        | Mouser P/N   | Note   |                |
|------------------|----------------------|---------------|----------------|--|--|----------------|
| C1,C3,C4, C13    | Capacitor            | 10 $\mu$ F    | 0805           |  | All capacitors have, at least, 10V rating.<br>All capacitors are ceramic layer type. |                |
| C10, C11         | Capacitor            | 1 $\mu$ F     | 0805           |  |  |                |
| C12              | Capacitor            | Not populated | 0805           |  |  |                |
| C2, C5, C8       | Capacitor            | 10nF          | 0805           |  |  |                |
| C6               | Capacitor            | 2.2nF         | 0805           |  |  |                |
| C7, C14          | Capacitor            | 100nF         | 0805           |  |  |                |
| C9               | Capacitor            | 4.7 $\mu$ F   | 0805           |  |  |                |
| D1               | LED, amber           |               | PLCC6          | 630-ASMT-QABD-AEF0E                                |  | Heartbeat Loss |
| D2               | LED, red             |               | PLCC6          | 630-ASMT-QRBD-AEF0E                                |  | Flash Detected |
| D3               | Schottky diode       |               | SMB            | 621-B240-F   | B240F  |                |
| D4               | LED, green           |               | 1206           | 630-HSMQ-C150                                      | External Heartbeat   |                |
| D5               | LED, blue            |               | 1206           | 630-HSMR-C150                                      | Internal Heartbeat   |                |
| D6               | Reference diode      |               | SOT23          | 700-LM4040DEM3-4.1T                                | LM4040-4.096V  |                |
| D7               | TVS diode            |               | DO-214AC       | 652-SMAJ5.0CA                                      | SMAJ5.0CA  |                |
| F1               | Polyfuse             | 300mA         | 2016           | 576-2016L030DR                                     | Resettable PTC   |                |
| JP1              | Header 2.54mm        |               | 100mil pitch   |  | Termination  |                |
| JP2              | Header 2.54mm        |               | 100mil pitch   |  | Operate-Measure  |                |
| L1               | Ferrite              |               | 0805           | 875-IC0805B182R-10                                 |  |                |
| M1               | Microcontroller      |               | 34-pin DIL     | 782-A000053  | Arduino Micro  |                |
| P5               | DC-Connector         |               | RASM722X       | 502-RASM722X                                       | 7.5 - 9 VDC Input  |                |
| P6               | RF-Connector SMA     |               | 5-pin SMA      | 571-5-1814832-1                                    | External Heartbeat Input   |                |
| Q1,Q2,Q3, Q4, Q5 | MOSFET N-Chan        |               | SOT23          | 512-2N7002   | 2N7002   |                |
| R1               | Resistor             | 39R           | 0805           |  | All resistors have a tolerance up to 1%<br>(E24 series), unless otherwise specified  |                |
| R10,R11          | Resistor             | 180R          | 1206           |  |  |                |
| R9, R12,R14      | Resistor             | 100k          | 0805           |  |  |                |
| R8,R13           | Resistor             | 24k           | 0805           |  |  |                |
| R15,R16          | Resistor             | 100R          | 1206           |  |  |                |
| R17,R18          | Resistor             | 270R          | 0805           |  |  |                |
| R2, R3, R19      | Resistor             | 510R          | 0805           |  |  |                |
| R20              | Resistor             | 0R            | 0805           |  |  |                |
| R21,R22          | Resistor             | 33R           | 0805           |  |  |                |
| R24,R25          | Resistor             | 3.9k          | 0805           |  |  |                |
| R4               | Resistor             | 130R          | 0805           |  |  |                |
| R5,R23           | Resistor             | Not populated | 0805           |  |  |                |
| R6               | Resistor             | 10k           | 0805           |  |  |                |
| R7               | Resistor             | 10R           | 1206           | 756-PCF1206R-10RBT1                                |  | 0.1% type      |
| RV1,RV2          | Potentiometer        | 5k            | T70YB-Series   | 72-T70YB-5K  |  |                |
| SW1              | TACT-Switch SMD      |               | SMD-Switch     | 101-0624-EV (switch button)<br>/ 101-0112-EV (cap) | Heartbeat select   |                |
| U1               | Voltage Regulator 5V |               | DPAK2          | 863-MC78M05CDTRKG                                  | MC78M05  |                |
| U2,U7            | IC, Monoflop         |               | SSOP8          | 595-SN74LVC1G123DCTR                               | 74LVC123   |                |
| U3               | Sensor Module        |               | AFBR-S10TR001Z |  | Avago Arc Flash Sensor Transceiver   |                |
| U4               | IC, NAND             |               | SSOP8          | 595-SN74LVC2G00DCTR                                | 74LVC2G00  |                |
| U5               | IC, Tristate buffer  |               | SSOP8          | 595-SN74LVC2G125DCTR                               | 74LVC125   |                |
| U6               | IC, AND              |               | SSOP8          | 595-SN74LVC2G08DCTR                                | 74LVC2G08  |                |
| W1               | Header 2.54mm        |               | 100mil pitch   |  | Tx Current Monitor   |                |
| W2               | Header 2.54mm        |               | 100mil pitch   |  | Threshold Voltage  |                |
| W3               | Header 2.54mm        |               | 100mil pitch   |  | Output Voltage   |                |

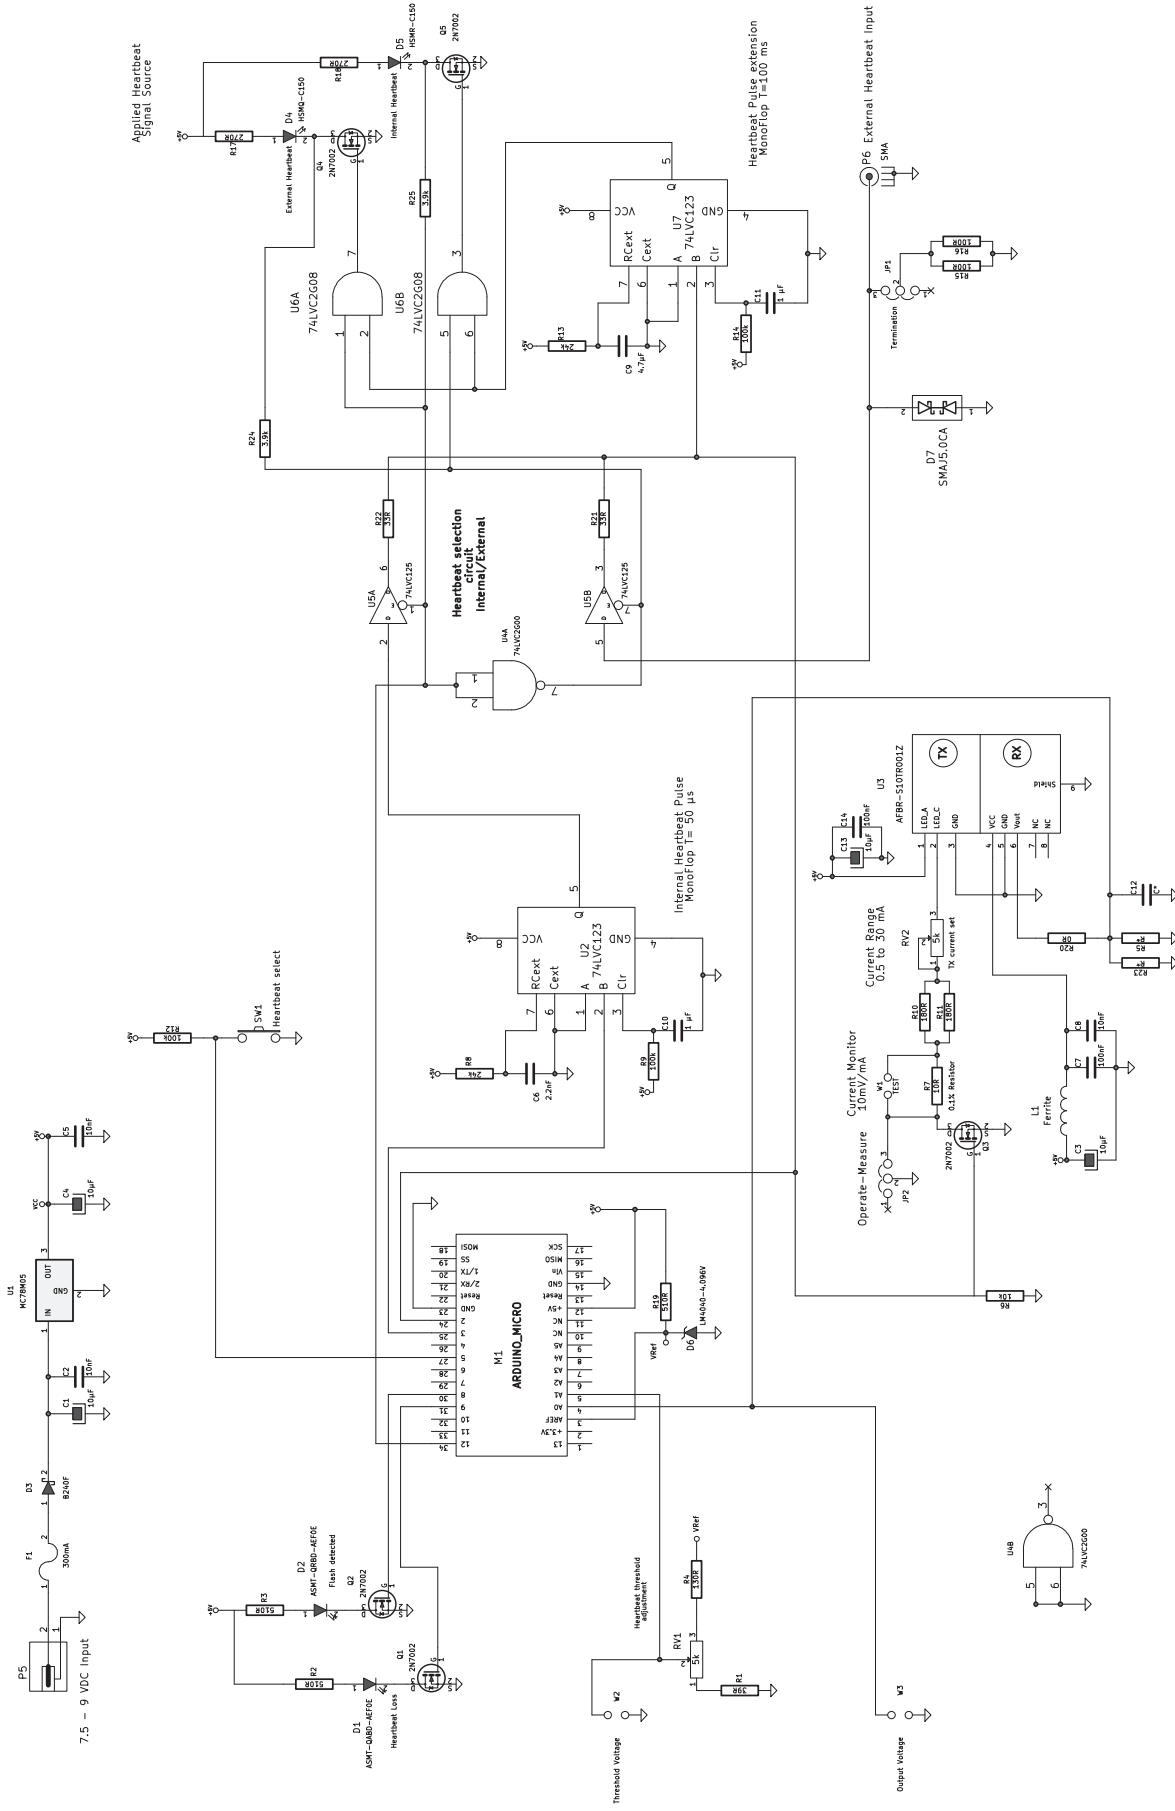


Figure 8. Schematic of the board included in the evaluation kit AFBR-S10EB001Z



For product information and a complete list of distributors, please go to our web site: [www.avagotech.com](http://www.avagotech.com)

Avago, Avago Technologies, and the A logo are trademarks of Avago Technologies in the United States and other countries.  
Data subject to change. Copyright © 2005-2015 Avago Technologies. All rights reserved.  
AV02-4913EN - May 8, 2015

